


Summary of the most commonly used test methods


Part 12 – Sterile hypodermic syringes (ISO 7886-1)

Sterile hypodermic syringes for manual use are tested according to ISO 7886-1.


- 13.1: Dead space (see also [Annex C](#))

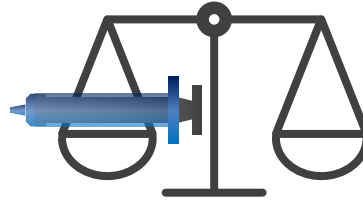


- 13.2: Freedom from air leakage past plunger stopper (see also [Annex B](#))

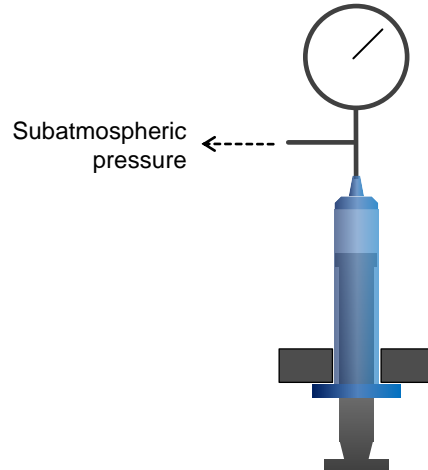

- 13.2: Freedom from liquid leakage past plunger stopper (see also [Annex D](#))

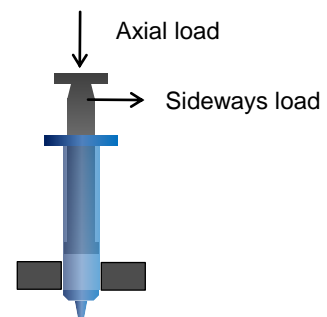

- 13.3: Force to operate the piston (see also [Annex E](#))

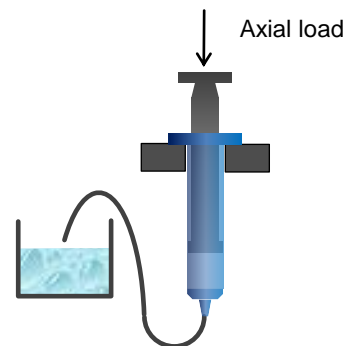

- 13.4: Fit of plunger stopper/plunger in barrel

For further information also regarding additional test methods not covered by this summary please contact:

SpineServ GmbH & Co. KG, Soefflinger Strasse 100, 89077 Ulm, Germany
 Phone: +49 (0)731 175 6788
 mail@spineserv.de
 www.spineserv.de